

# Surgical Technique

## Fortilink<sup>®</sup>-A *with TiPlus Technology*

Document name: 19031\_Surgical\_Technique\_EU\_A\_rev2

Date of issue: 2022-08-04

Revision number: 2



### Manufacturer



BAAT Medical Products BV  
F. Hazemeijerstraat 800  
7555 RJ Hengelo  
The Netherlands  
+31 (0)88 565 66 00  
[www.baatmedical.com](http://www.baatmedical.com)

### Distributor



Surgalign Spine Technologies, Inc.  
520 Lake Cook Rd, Suite 315  
Deerfield, IL 60015  
United States of America  
+1 844.894.7752  
[www.surgalign.com](http://www.surgalign.com)

## Contents

1.	Introduction.....	3
1.1.	Device description .....	3
1.2.	Intended purpose .....	3
1.3.	Clinical benefits.....	4
1.4.	Indications.....	4
1.5.	Contraindications.....	4
1.6.	Sterility.....	4
1.7.	Material specification .....	4
1.8.	Warnings and precautions.....	5
1.9.	Potential adverse effects .....	9
2.	Surgical technique .....	10
2.1.	Patient positioning.....	10
2.2.	Exposure of disc level .....	10
2.3.	Discectomy and endplate preparation .....	10
2.4.	Distraction.....	11
2.5.	Implant selection .....	11
2.6.	Implant preparation.....	12
2.7.	Insertion preparation .....	12
2.8.	Insertion assembly.....	12
2.9.	Insertion and implant loading .....	13
2.10.	Radiographic verification .....	15
2.11.	Fixation options .....	15
2.12.	Removal (if necessary).....	15
3.	Catalogue implants.....	16
4.	Catalogue instruments .....	18

# 1. Introduction

## 1.1. Device description

The Fortilink-A Ti (*Figure 1*) is an interbody fusion device intended for the lumbar spine (L2-S1) in patients with degenerative disc diseases. The Fortilink-A Ti interbody fusion devices are manufactured with SLM (selective laser melting) and are built up from implant grade titanium alloy (Ti6Al4V). The Fortilink-A Ti has an open mesh structure and a bone window both designed to allow bone ingrowth and facilitate fusion. The box-shaped design is intended to provide primary stability and increase the intervertebral height and lordosis.

The Fortilink-A Ti will be used in combination with:

- Dedicated instrument set (see surgical technique for Catalogue Instruments)
- General instruments typically used in spinal surgery (including rongeurs, forceps)

Further copies of the surgical technique and instructions for use can be requested at BAAT Medical Products BV.



Figure 1. Fortilink®-A with TiPlus Technology

## 1.2. Intended purpose

The Fortilink-A Ti is indicated for anterior interbody fusion (IBF) of the spine in skeletally mature patients with degenerative disc disease (DDD) and up to Grade 1 spondylolisthesis of the lumbar spine at one level or two contiguous levels. DDD is defined as back pain of discogenic origin with degeneration of the disc confirmed by history and radiographic studies. These IBF devices are used to facilitate interbody fusion in the lumbar spine from L2 to S1 using autogenous bone graft and/or allogenic bone graft comprised of cancellous and/or corticocancellous bone graft to facilitate fusion. The IBF devices are intended to be used with supplemental fixation designed for the implanted level. Patients should have at least six months of non-operative treatment prior to treatment with an interbody fusion device. Hyperlordotic interbody devices ( $\geq 20^\circ$  lordosis) must be used with at least anterior supplemental fixation.

### **1.3. Clinical benefits**

The following benefits to the patient are intended to be achieved with the Fortilink-A Ti:

- Decrease back pain, as assessed using the Visual Analogue Scale (VAS)
- Clinical improvement, as assessed using the Oswestry Disability Index (ODI)
- Facilitate fusion, assessed by fusion rates in radiological follow-up images
- Increase in intervertebral height, as measured by increase in post-operative disc height on radiological imaging.
- Increase in lordosis, as measured by increase in post-operative lordosis on radiological imaging

### **1.4. Indications**

Degenerative disc disease (DDD) and up to Grade 1 spondylolisthesis of the lumbar spine at one level or two contiguous levels. DDD is defined as back pain of discogenic origin with degeneration of the disc confirmed by history and radiographic studies.

### **1.5. Contraindications**

- Active systemic infection or an active infection at the operative site
- A demonstrated allergy or sensitivity to any of the implant materials
- Severe osteoporosis
- Primary or metastatic tumors affecting the spine
- Conditions that may place excessive stresses on bones and the implants, including but not limited to morbid obesity, or other degenerative diseases
- Patients whose ability to follow postoperative restrictions, precautions and rehabilitation programs is limited
- Fractures, severe deformities or a severe instability in the area of surgery
- A medical or surgical situation that would preclude the benefit of surgery
- Pregnancy

### **1.6. Sterility**

The implant is delivered sterile packed. The devices are sterilized by irradiation. Do not re-use or re-sterilize the implants in this system, as adequate mechanical performance, biocompatibility and sterility cannot be guaranteed.

### **1.7. Material specification**

The implants are manufactured from implant grade titanium alloy Ti6Al4V ELI (ASTM F3001).



## 1.8. Warnings and precautions

<p><b>INTENDED USERS</b></p> <p>Prior to use the surgeon must become familiar with the device system and the surgical procedure. Use surgical instrumentation, accessories, and surgical technique guide provided with this device system. The implantation of the IBF device should be performed only by experienced spinal surgeons with specific training in the use of this device because this is a technically demanding procedure presenting a risk of serious injury to the patient.</p>
<p><b>PATIENT EDUCATION</b></p> <p><u>Preoperative</u></p> <p>The patient should understand that stress on an implant could involve more than weight bearing. In the absence of solid bony union, patient weight alone, muscular forces associated with moving, or repeated stresses of apparent relatively small magnitude, can compromise the implant. Patients should be fully informed of these risks prior to and following surgery.</p> <p><u>Postoperative</u></p> <p>The surgeon should provide clear directions, warnings and must obtain verification of patient understanding for patient post-operative compliance.</p> <ul style="list-style-type: none"> <li>• Partial- or non-weight bearing may be recommended or required to achieve firm bone union.</li> <li>• Warn patient against smoking, consuming alcohol, and/or taking steroids, non-steroidal anti-inflammatory agents and aspirin or other drugs not prescribed by the physician.</li> <li>• Warn patient against sudden changes in position, strenuous activity or falls that may cause additional injury and advice that the patient seek medical opinion before entering environments in which this might occur.</li> <li>• Warn patient to consult the surgeon in the event of malfunction of the device or changes in its performance that may affect safety.</li> <li>• If appropriate, restrict patient's mobility to allow bony union.</li> <li>• If nonunion occurs, the surgeon may revise or remove the system.</li> </ul>
<p><b>READ THE INSTRUCTIONS</b></p> <p>All users are expected to read the instructions for use that accompany all devices being utilized with these implants.</p>
<p><b>PATIENT SELECTION</b></p> <ul style="list-style-type: none"> <li>• Avoid patients not meeting the criteria described in the indications.</li> <li>• Avoid patients with conditions that may predispose to a possible poor result or adverse effect.</li> </ul>
<p><b>IMPACT RISK</b></p> <p>No implant system can withstand the forces of sudden dynamic loads such as falls or other accidents.</p>
<p><b>SINGLE USE ONLY</b></p> <p>Do not re-use or re-sterilize the implants in this system, as adequate mechanical performance, biocompatibility and sterility cannot be guaranteed.</p>
<p><b>MIXING WITH OTHER DEVICES</b></p> <p>Mixing of implant components with different materials is not recommended, for metallurgical, mechanical and functional reasons.</p>
<p><b>INSTRUMENTS</b></p> <p>Only use instruments and accessories listed in the surgical technique to avoid adversely affecting device performance or surgical outcome. Surgeons must verify that the instruments are in good condition and in operating order prior to use during surgery.</p>

***INSERTION INSTRUMENTS***

For implant insertion, use only the instruments provided. Using other instruments to insert the implant could result in implant damage.

***CLEANING AND STERILIZATION***

Implants are provided sterile. Reusable instruments are provided non-sterile. For specific cleaning and sterilization instructions, refer to the instructions for use provided with the device or contact the distributor.

***PACKAGING INTEGRITY***

Inspect the product, including all packaging and labeling materials carefully:

- Do not use past expiration date specified on the product label.
- Do not use if the implant or packaging is damaged or unintentionally opened before use.
- Do not use if there are discrepancies in label information.

***DISC SPACE PREPARATION***

Care should be taken to avoid pushing the shaver too far in the interspace and cutting through the annulus.

Care should be taken when first rotating the shavers to not force them into the bony endplates, increasing the risk of subsidence. If the shaver catches, drop down one size and proceed.

***ENDPLATE PREPARATION***

Appropriate removal of the cartilaginous layers of the endplates is important for the vascularization of the bone graft. However, make sure to clean the endplates carefully and maintain the integrity of the underlying bony endplate, as damage of the endplate can lead to implant subsidence.

***DISTRACTION***

Adequate distraction is one of the preconditions for the primary stability of the implant; it is critical to ensure that the segment is not over distracted to avoid damage of ligaments and/or endplates.

***SIZE SELECTION***

Select the trial spacer that adequately fills the disc space and provides restoration of disc height.

The trial spacer should require minimal force to insert, yet fit snugly within the disc space.

Sequentially increase the trial spacer size until the appropriate height is determined. Using the trial spacer as a guide, verify that appropriate height restoration is achieved with lateral fluoroscopy.

Select the appropriate implant size.

Using an implant smaller or larger than the size trialed could lead to implant failure.

Preoperative planning and patient anatomy should be considered when selecting implant size and supplemental internal fixation. The physician should consider the levels of implantation, patient weight, patient activity level, and other patient conditions which may impact the performance of the device.

***SIZE CORRESPONDANCE***

The relation of the size of the trial spacers to the size of the implants must be taken into account.

***PRODUCT AVAILABILITY***

It must be ascertained that the implant is available in all sizes in the range that is appropriate for the patient before starting the procedure in order to make sure that the optimal size, which is determined intraoperatively with the trial sizers, will be available.

<p><b><i>IMPLANT PLACEMENT</i></b></p> <p>The cage has teeth to maximize primary stability, however make sure the soft tissue and dura are adequately retracted when inserting the implant to avoid damage from contact with the cage (in particular the teeth). Adequate implant positioning is critical; an improperly placed implant can adversely affect device performance or surgical outcome.</p>
<p><b><i>SUPPLEMENTAL FIXATION</i></b></p> <p>Interbody fusion devices are designed to withstand full load-bearing until bony union of the spinal segment(s) normally occurs. To ensure load-bearing capability, supplemental fixation is required for use with these devices. Hyperlordotic interbody devices (<math>\geq 20^\circ</math> lordosis) must be used with at least anterior supplemental fixation.</p>
<p><b><i>LOAD-BEARING</i></b></p> <p>While proper selection can help minimize risks, the size and shape of human bones present limitations on the size, shape, and strength of implants. Internal fixation devices cannot withstand activity levels equal to those placed on normal healthy bone.</p> <p>These implants can break when subjected to the increased loading associated with delayed union or nonunion. Typically, internal fixation devices are load-sharing devices which hold a fracture in alignment until healing occurs. If healing is delayed, or does not occur, an implant could eventually break due to fatigue. Loads produced by weight bearing and activity levels will dictate the longevity of the implant.</p>
<p><b><i>EXPLANTATION</i></b></p> <p>After implantation of an interbody fusion device and identification of the presence of fusion, only the supplemental fixation components should be removed.</p>
<p><b><i>COMORBIDITIES</i></b></p> <p>Certain degenerative diseases or underlying physiological conditions such as diabetes or rheumatoid arthritis may alter the healing process, thereby increasing the risk of implant breakage.</p>
<p><b><i>PREVIOUS SURGERY</i></b></p> <p>Patients with previous spinal surgery at the level(s) to be treated may have different clinical outcomes compared to those without a previous surgery.</p>
<p><b><i>INSTRUMENT WEAR</i></b></p> <p>Instruments are subject to damage during use as well as long-term potentially damaging effects such as wear. Damage may result in significant risks to safety and/or inability to function as intended.</p>
<p><b><i>INSTRUMENT FRAGMENTS</i></b></p> <p>If instruments are damaged or broken during use, metal fragments can be viewed by radiographic assessment. It is the surgeon's responsibility to carefully consider the risks and benefits of retrieving the fragments.</p> <p>If the fragment is retained in the patient, it is recommended that the surgeon advise the patient of specific information regarding the fragment material, including size and location and the potential risks associated with the retained fragment.</p>
<p><b><i>IMPLANT HANDLING</i></b></p> <p>Correct handling of the implant is extremely important. Alterations will produce internal stresses which may lead to eventual breakage of the implant. An explanted implant should never be re-implanted. Even though the implant appears undamaged, it may have small defects and internal stress patterns which may lead to early breakage.</p>
<p><b><i>RADIOGRAPHIC VERIFICATION</i></b></p> <p>Verify the final implant placement with anterior/posterior and lateral fluoroscopy images.</p>

**MRI SAFETY INFORMATION**

A patient with this device can be safely scanned in an MR system meeting the following conditions:

- Static magnetic field of 1.5-Tesla (1.5 T) or 3-Tesla (3 T).
- Maximum spatial gradient magnetic field of 720-Gauss/cm (a higher value for the spatial gradient magnetic field may apply if properly calculated).
- Maximum MR system reported whole-body-averaged specific absorption rate (SAR) of 2-W/kg for 15 minutes of scanning (per pulse sequence).

**RF Heating**

In non-clinical testing, the device can produce a temperature rise of less than or equal to 6.0 degrees C using an MR system reported, whole body averaged specific absorption rate (SAR) of 2-W/kg for 15-minutes (per pulse sequence) of scanning in a 3-Tesla MR system.

The RF heating behavior does not scale with static field strength. Devices that do not exhibit detectable heating at one field strength may exhibit high values of localized heating at another field strength.

**Artifact**

MR image quality may be compromised if the area of interest is in the exact same area or relatively close to the position of the device.

In all cases, the healthcare professional is responsible for the MR conditions, MR imaging quality and patient safety. Any safety issues or major image artefacts should be reported.

**DISPOSAL**

The products must be disposed according to local regulations.



## **1.9. Potential adverse effects**

The same medical/surgical conditions or complications that apply to any surgical procedure may also occur during or following implantation of this device system. The surgeon is responsible for informing the patient of the potential risks associated with treatment, including complications and adverse reactions. The surgeon may need to perform additional surgery to address any complications or adverse reactions, which may or may not be device related.

Potential risks identified with the use of this intervertebral body fusion device, which may require additional surgery include:

- Implant component fracture
- Migration, dislocation, or subsidence of the implant
- Loss of fixation
- Pseudoarthrosis (i.e., non-union)
- Fracture of the vertebra
- Neurological injury
- Cardiovascular complications
- Visceral injury
- Retrograde ejaculation
- Infection
- Allergic reaction
- Pulmonary embolism
- Pneumonia
- Adjacent segment disease
- Heterotrophic ossification
- Bone erosion
- Epidural scarring
- Ureter damage

## 2. Surgical technique

### 2.1. Patient positioning

The patient should be placed in a supine position appropriate for an anterior approach. For anterior approach to the lower lumbar levels, position the patient in a slight Trendelenburg position.

### 2.2. Exposure of disc level

Locate the correct operative disc level and make an incision location by taking a lateral X-ray (fluoroscopic view) while holding a straight metal instrument at the side of the patient (*Figure 2*). This ensures that the incision and exposure will allow direct visualization into the disc space. Expose the operative disc level and retract tissues using appropriate instrumentation. Retract and protect the great vessels to allow complete exposure and visualization of the operative site.



Figure 2

### 2.3. Discectomy and endplate preparation

Perform a complete discectomy using appropriate instrumentation.



#### *INSTRUMENTS*

Only use instruments and accessories listed in the surgical technique to avoid adversely affecting device performance or surgical outcome. Surgeons must verify that the instruments are in good condition and in operating order prior to use during surgery.



#### *DISC SPACE PREPARATION*

Care should be taken to avoid pushing the shaver too far in the interspace and cutting through the annulus.

Care should be taken when first rotating the shavers to not force them into the bony endplates, increasing the risk of subsidence. If the shaver catches, drop down one size and proceed.



#### *ENDPLATE PREPARATION*

Appropriate removal of the cartilaginous layers of the endplates is important for the vascularization of the bone graft. However, make sure to clean the endplates carefully and maintain the integrity of the underlying bony endplate, as damage of the endplate can lead to implant subsidence.

## 2.4. Distraction

Spreaders may be used to distract the disc space. A smaller width of the spreader may be inserted first to aid in distraction of the disc space. After initial distraction, turn the spreader 90 degrees to the full spreader height to distract the disc space.



### *DISTRACTION*

Adequate distraction is one of the preconditions for the primary stability of the implant; it is critical to ensure that the segment is not over distracted to avoid damage of ligaments and/or endplates.

## 2.5. Implant selection

Trial spacers are available to provide guidance prior to implant selection. For an overview of the available trial spacers, see 'Catalogue instruments'.



### *SIZE SELECTION*

Select an appropriate size detachable trial head and assemble it to the trial shaft handle by threading the trial handle clockwise until the positive stop is reached (*Figure 3*). Trial markings indicate footprint size, height and angle of lordosis. The trial spacer should require minimum force to insert yet fit snugly within the disc space (*Figure 4*). Sequentially increase the trial spacer size until the appropriate fit is determined. Using the trial spacer as a guide, verify that appropriate height restoration is achieved with lateral fluoroscopy. Select the appropriate implant size.

Using an implant smaller or larger than the size trialed could lead to implant failure.

Preoperative planning and patient anatomy should be considered when selecting implant size and supplemental internal fixation. The physician should consider the levels of implantation, patient weight, patient activity level, and other patient conditions which may impact the performance of the device.



**Figure 3**



**Figure 4**

Insert the trial into the annulotomy window. Check fit and positioning with anterior/posterior (A/P) and lateral fluoroscopy. Repeat until the desired fit is achieved to identify the optimal trial profile.

## 2.6. Implant preparation

Select the implant based upon the trial sizing. The Fortilink-A trials are sized line-to-line to the implant. The implants are available in different lordotic degrees and sizes, see 'Catalogue Implants'.

Pack the implant with autogenous and/or allogenic bone graft comprised of cancellous and/or corticocancellous bone graft.

## 2.7. Inserter preparation

Both anterolateral and straight inserters are available to aid with insertion for specific approaches (*Figure 5*). Each inserter type has their specific inner shaft and external housing.

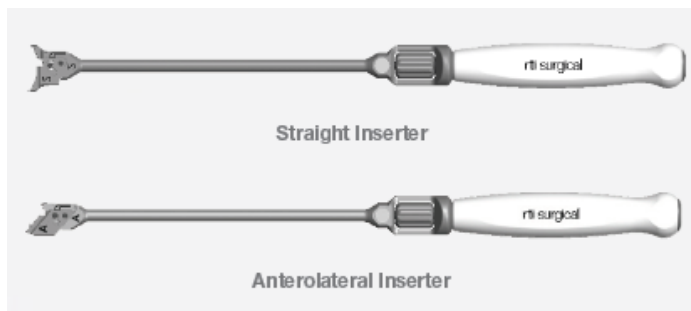


Figure 5

## 2.8. Inserter assembly

To assemble, insert the inner shaft into the housing (*Figure 6A*), depress the button (*Figure 6B*) and push shaft within housing until a positive stop is felt. With the jaws facing you, align the inner shaft jaw flat and housing jaw flat (*Figure 7*), rotate the knob clockwise until the shaft is fully seated (*Figure 6C*).

Verify the labeling on the inner shaft is the same when assembling to the housing ("S" indicates straight inserter and "A" indicates the anterolateral inserter).

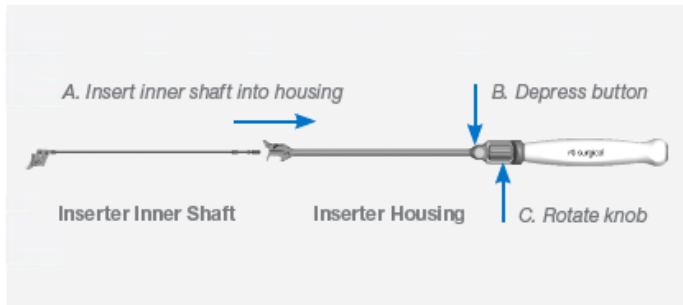


Figure 6

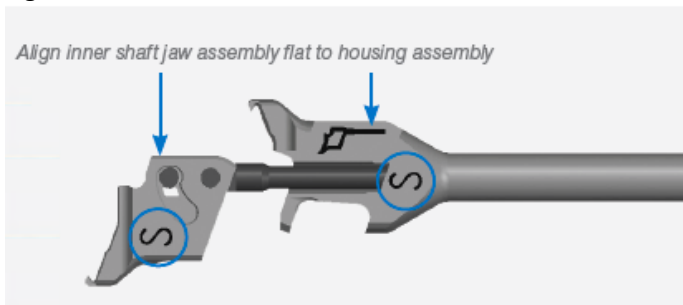


Figure 7

## 2.9. Inserter and implant loading

Rotate inserter knob counterclockwise until positive stop is felt, visually confirm distal end is fully open (*Figure 8*).

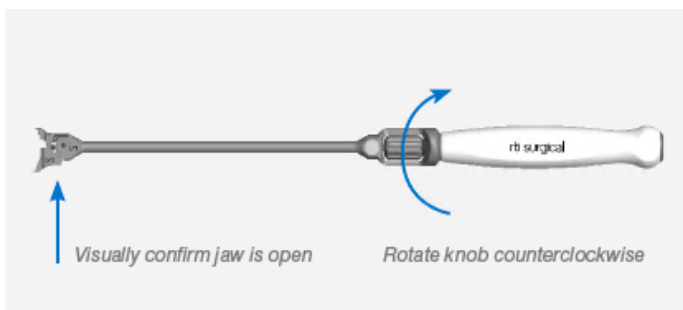
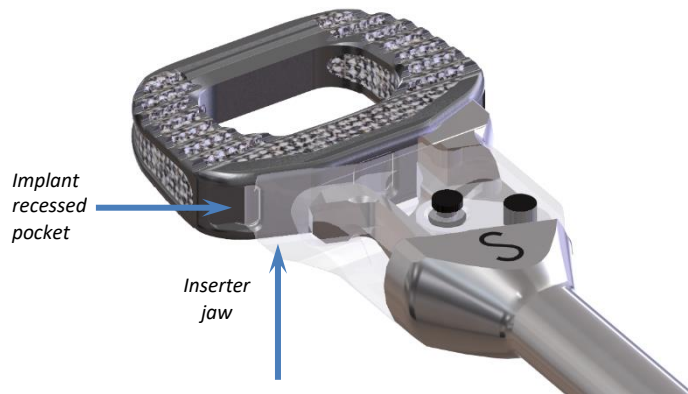


Figure 8

Attach the selected implant to the inserter by placing the inserter jaw into the recessed implant pocket (*Figure 9*). Rotate the knob clockwise until a positive stop is reached. Verify the implant is fully attached to inserter before inserting into the disc space (*Figure 10*). Insert the implant into the desired position as determined by direct visualized and lateral fluoroscopy.

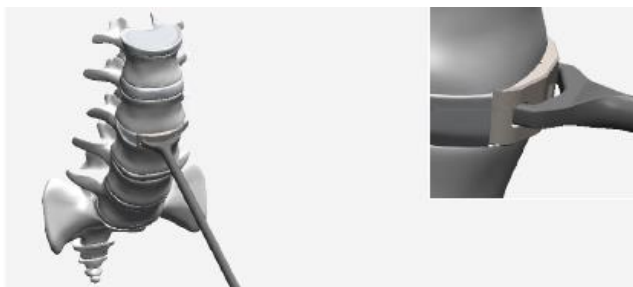


**Figure 9**



**Figure 10**

If fine adjustments are needed for final placement of the implant, the tamp may be used to aid in final positioning of the implant (*Figure 11*). When using the tamp, always ensure that it is docked within the inserter geometry for direct tamping and if corner tamping is required, ensure that the cup portion of the tamp is at the corner of the implant. Always use gentle force when tamping.



**Figure 11**



**INSERTION INSTRUMENTS**

For implant insertion, use only the instruments provided. Using other instruments to insert the implant could result in implant damage.



**IMPLANT PLACEMENT**

The cage has teeth to maximize primary stability, however make sure the soft tissue and dura are adequately retracted when inserting the implant to avoid damage from contact with the cage (in particular the teeth). Adequate implant positioning is critical; an improperly placed implant can adversely affect device performance or surgical outcome.

## 2.10. Radiographic verification



### *RADIOGRAPHIC VERIFICATION*

Verify the final implant placement with anterior/posterior and lateral fluoroscopy images.

## 2.11. Fixation options



### *SUPPLEMENTAL FIXATION*

Interbody fusion devices are designed to withstand full load-bearing until bony union of the spinal segment(s) normally occurs. To ensure load-bearing capability, supplemental fixation is required for use with these devices. Hyperlordotic interbody devices ( $\geq 20^\circ$  lordosis) must be used with at least anterior supplemental fixation.

## 2.12. Removal (if necessary)

Assemble the inner jaw to the housing. After assembly (see previous steps), re-engage inserter to the implant. Rotate knob of inserter clockwise for reattachment until positive stop is felt. Attach slap hammer adapter to the inserter. Assemble slap hammer to the slap hammer attachment. Carefully back slap the hammer and remove the implant from the disc space.

### 3. Catalogue implants

Product number	Product name	Width (mm)	Length (mm)	Height (mm)	Lordosis (°)	Quantity
77-A-3225-08-8L	Fortilink-A Ti 32x25x08-8L	32	25	8	8	1
77-A-3225-10-8L	Fortilink-A Ti 32x25x10-8L	32	25	10	8	1
77-A-3225-12-8L	Fortilink-A Ti 32x25x12-8L	32	25	12	8	1
77-A-3225-14-8L	Fortilink-A Ti 32x25x14-8L	32	25	14	8	1
77-A-3225-16-8L	Fortilink-A Ti 32x25x16-8L	32	25	16	8	1
77-A-3225-18-8L	Fortilink-A Ti 32x25x18-8L	32	25	18	8	1
77-A-3225-10-14L	Fortilink-A Ti 32x25x10-14L	32	25	10	14	1
77-A-3225-12-14L	Fortilink-A Ti 32x25x12-14L	32	25	12	14	1
77-A-3225-14-14L	Fortilink-A Ti 32x25x14-14L	32	25	14	14	1
77-A-3225-16-14L	Fortilink-A Ti 32x25x16-14L	32	25	16	14	1
77-A-3225-18-14L	Fortilink-A Ti 32x25x18-14L	32	25	18	14	1
77-A-3225-12-20L	Fortilink-A Ti 32x25x12-20L	32	25	12	20	1
77-A-3225-14-20L	Fortilink-A Ti 32x25x14-20L	32	25	14	20	1
77-A-3225-16-20L	Fortilink-A Ti 32x25x16-20L	32	25	16	20	1
77-A-3225-18-20L	Fortilink-A Ti 32x25x18-20L	32	25	18	20	1
77-A-3225-20-20L	Fortilink-A Ti 32x25x20-20L	32	25	20	20	1
77-A-3225-16-30L	Fortilink-A Ti 32x25x16-30L	32	25	16	30	1
77-A-3225-18-30L	Fortilink-A Ti 32x25x18-30L	32	25	18	30	1
77-A-3225-20-30L	Fortilink-A Ti 32x25x20-30L	32	25	20	30	1
77-A-3225-22-30L	Fortilink-A Ti 32x25x22-30L	32	25	22	30	1
77-A-3627-08-8L	Fortilink-A Ti 36x27x08-8L	36	27	8	8	1
77-A-3627-10-8L	Fortilink-A Ti 36x27x10-8L	36	27	10	8	1
77-A-3627-12-8L	Fortilink-A Ti 36x27x12-8L	36	27	12	8	1
77-A-3627-14-8L	Fortilink-A Ti 36x27x14-8L	36	27	14	8	1
77-A-3627-16-8L	Fortilink-A Ti 36x27x16-8L	36	27	16	8	1
77-A-3627-18-8L	Fortilink-A Ti 36x27x18-8L	36	27	18	8	1
77-A-3627-10-14L	Fortilink-A Ti 36x27x10-14L	36	27	10	14	1
77-A-3627-12-14L	Fortilink-A Ti 36x27x12-14L	36	27	12	14	1
77-A-3627-14-14L	Fortilink-A Ti 36x27x14-14L	36	27	14	14	1
77-A-3627-16-14L	Fortilink-A Ti 36x27x16-14L	36	27	16	14	1
77-A-3627-18-14L	Fortilink-A Ti 36x27x18-14L	36	27	18	14	1
77-A-3627-14-20L	Fortilink-A Ti 36x27x14-20L	36	27	14	20	1
77-A-3627-16-20L	Fortilink-A Ti 36x27x16-20L	36	27	16	20	1
77-A-3627-18-20L	Fortilink-A Ti 36x27x18-20L	36	27	18	20	1
77-A-3627-20-20L	Fortilink-A Ti 36x27x20-20L	36	27	20	20	1
77-A-3627-18-30L	Fortilink-A Ti 36x27x18-30L	36	27	18	30	1
77-A-3627-20-30L	Fortilink-A Ti 36x27x20-30L	36	27	20	30	1



Product number	Product name	Width (mm)	Length (mm)	Height (mm)	Lordosis (°)	Quantity
77-A-3627-22-30L	Fortilink-A Ti 36x27x22-30L	36	27	22	30	1
77-A-4029-08-8L	Fortilink-A Ti 40x29x08-8L	40	29	8	8	1
77-A-4029-10-8L	Fortilink-A Ti 40x29x10-8L	40	29	10	8	1
77-A-4029-12-8L	Fortilink-A Ti 40x29x12-8L	40	29	12	8	1
77-A-4029-14-8L	Fortilink-A Ti 40x29x14-8L	40	29	14	8	1
77-A-4029-16-8L	Fortilink-A Ti 40x29x16-8L	40	29	16	8	1
77-A-4029-18-8L	Fortilink-A Ti 40x29x18-8L	40	29	18	8	1
77-A-4029-12-14L	Fortilink-A Ti 40x29x12-14L	40	29	12	14	1
77-A-4029-14-14L	Fortilink-A Ti 40x29x14-14L	40	29	14	14	1
77-A-4029-16-14L	Fortilink-A Ti 40x29x16-14L	40	29	16	14	1
77-A-4029-18-14L	Fortilink-A Ti 40x29x18-14L	40	29	18	14	1
77-A-4029-14-20L	Fortilink-A Ti 40x29x14-20L	40	29	14	20	1
77-A-4029-16-20L	Fortilink-A Ti 40x29x16-20L	40	29	16	20	1
77-A-4029-18-20L	Fortilink-A Ti 40x29x18-20L	40	29	18	20	1
77-A-4029-20-20L	Fortilink-A Ti 40x29x20-20L	40	29	20	20	1
77-A-4029-18-30L	Fortilink-A Ti 40x29x18-30L	40	29	18	30	1
77-A-4029-20-30L	Fortilink-A Ti 40x29x20-30L	40	29	20	30	1
77-A-4029-22-30L	Fortilink-A Ti 40x29x22-30L	40	29	22	30	1

## 4. Catalogue instruments

Instruments are manufactured by Pioneer Surgical Technology Inc. and distributed by Surgalign Spine Technologies, Inc.

Instrument list Fortilink-A Ti (ALIF)	
Part #	Description
65-ACE-TAMP	Fortilink-A, Tamp
65-ACE-INSERTR-TRL	Trial Shaft
65-ACE-INSERTER	Fortilink-A, Straight Inserter
65-ACE-SHAFT	Fortilink-A, Straight Jaw Shaft
65-ACE-INSERTER-A	Fortilink-A, Anterolateral Inserter
65-ACE-SHAFT-A	Fortilink-A, Anterolateral Jaw Shaft
65-ACE-S08-8L-TRL	Fortilink-A, 32x25x08x8L-TRL
65-ACE-S10-8L-TRL	Fortilink-A, 32x25x10x8L-TRL
65-ACE-S12-8L-TRL	Fortilink-A, 32x25x12x8L-TRL
65-ACE-S14-8L-TRL	Fortilink-A, 32x25x14x8L-TRL
65-ACE-S16-8L-TRL	Fortilink-A, 32x25x16x8L-TRL
65-ACE-S18-8L-TRL	Fortilink-A, 32x25x18x8L-TRL
65-ACE-S10-14L-TRL	Fortilink-A, 32x25x10x14L-TRL
65-ACE-S12-14L-TRL	Fortilink-A, 32x25x12x14L-TRL
65-ACE-S14-14L-TRL	Fortilink-A, 32x25x14x14L-TRL
65-ACE-S16-14L-TRL	Fortilink-A, 32x25x16x14L-TRL
65-ACE-S18-14L-TRL	Fortilink-A, 32x25x18x14L-TRL
65-ACE-S12-20L-TRL	Fortilink-A, 32x25x12x20L-TRL
65-ACE-S14-20L-TRL	Fortilink-A, 32x25x14x20L-TRL
65-ACE-S16-20L-TRL	Fortilink-A, 32x25x16x20L-TRL
65-ACE-S18-20L-TRL	Fortilink-A, 32x25x18x20L-TRL
65-ACE-S20-20L-TRL	Fortilink-A, 32x25x20x20L-TRL
65-ACE-S16-30L-TRL	Fortilink-A, 32x25x16x30L-TRL
65-ACE-S18-30L-TRL	Fortilink-A, 32x25x18x30L-TRL
65-ACE-S20-30L-TRL	Fortilink-A, 32x25x20x30L-TRL
65-ACE-S22-30L-TRL	Fortilink-A, 32x25x22x30L-TRL
65-ACE-M08-8L-TRL	Fortilink-A, 36x27x08x8L-TRL
65-ACE-M10-8L-TRL	Fortilink-A, 36x27x10x8L-TRL
65-ACE-M12-8L-TRL	Fortilink-A, 36x27x12x8L-TRL
65-ACE-M14-8L-TRL	Fortilink-A, 36x27x14x8L-TRL
65-ACE-M16-8L-TRL	Fortilink-A, 36x27x16x8L-TRL
65-ACE-M18-8L-TRL	Fortilink-A, 36x27x18x8L-TRL
65-ACE-M10-14L-TRL	Fortilink-A, 36x27x10x14L-TRL
65-ACE-M12-14L-TRL	Fortilink-A, 36x27x12x14L-TRL
65-ACE-M14-14L-TRL	Fortilink-A, 36x27x14x14L-TRL

<b>Instrument list Fortilink-A Ti (ALIF)</b>	
<b>Part #</b>	<b>Description</b>
65-ACE-M16-14L-TRL	Fortilink-A, 36x27x16x14L-TRL
65-ACE-M18-14L-TRL	Fortilink-A, 36x27x18x14L-TRL
65-ACE-M14-20L-TRL	Fortilink-A, 36x27x14x20L-TRL
65-ACE-M16-20L-TRL	Fortilink-A, 36x27x16x20L-TRL
65-ACE-M18-20L-TRL	Fortilink-A, 36x27x18x20L-TRL
65-ACE-M20-20L-TRL	Fortilink-A, 36x27x20x20L-TRL
65-ACE-M18-30L-TRL	Fortilink-A, 36x27x18x30L-TRL
65-ACE-M20-30L-TRL	Fortilink-A, 36x27x20x30L-TRL
65-ACE-M22-30L-TRL	Fortilink-A, 36x27x22x30L-TRL
65-ACE-L08-8L-TRL	Fortilink-A, 40x29x08x8L-TRL
65-ACE-L10-8L-TRL	Fortilink-A, 40x29x10x8L-TRL
65-ACE-L12-8L-TRL	Fortilink-A, 40x29x12x8L-TRL
65-ACE-L14-8L-TRL	Fortilink-A, 40x29x14x8L-TRL
65-ACE-L16-8L-TRL	Fortilink-A, 40x29x16x8L-TRL
65-ACE-L18-8L-TRL	Fortilink-A, 40x29x18x8L-TRL
65-ACE-L12-14L-TRL	Fortilink-A, 40x29x12x14L-TRL
65-ACE-L14-14L-TRL	Fortilink-A, 40x29x14x14L-TRL
65-ACE-L16-14L-TRL	Fortilink-A, 40x29x16x14L-TRL
65-ACE-L18-14L-TRL	Fortilink-A, 40x29x18x14L-TRL
65-ACE-L14-20L-TRL	Fortilink-A, 40x29x14x20L-TRL
65-ACE-L16-20L-TRL	Fortilink-A, 40x29x16x20L-TRL
65-ACE-L18-20L-TRL	Fortilink-A, 40x29x18x20L-TRL
65-ACE-L20-20L-TRL	Fortilink-A, 40x29x20x20L-TRL
65-ACE-L18-30L-TRL	Fortilink-A, 40x29x18x30L-TRL
65-ACE-L20-30L-TRL	Fortilink-A, 40x29x20x30L-TRL
65-ACE-L22-30L-TRL	Fortilink-A, 40x29x22x30L-TRL